


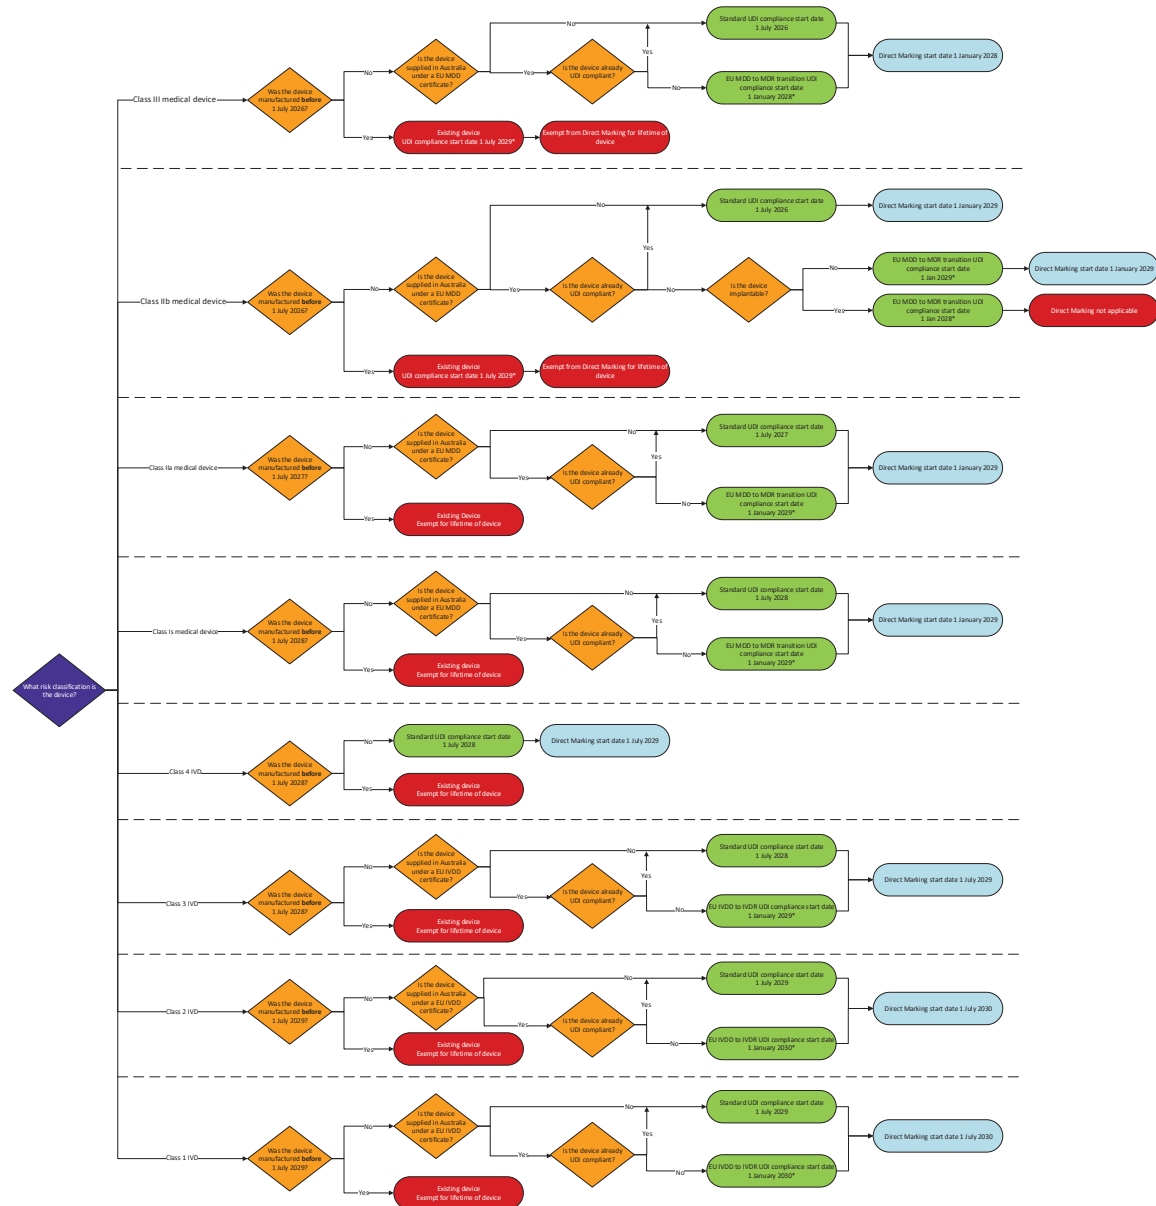

*If a device eligible a transitional arrangement becomes UDI compliant before the transitional compliance date, it must meet Australia's UDI requirements from the date it becomes UDI compliant. For example, if a device transitions to EU MDR or IVDR **after** the standard UDI compliance date but **before** the EU MDD to MDR or EU IVDD to IVDR UDI compliance start dates, the device must meet Australian UDI requirements from the date it has transitioned. If an existing device is relabelled after the standard UDI compliance date but before its transitional date, it must comply with UDI requirements at the time of relabelling.