

Flowflex™ SARS-CoV-2 Antigen Rapid Test (Self-Testing)

Package Insert

REF L031-118M5 REF L031-118P5 REF L031-118Z5 English

A rapid test for the detection of SARS-CoV-2 nucleocapsid antigens in anterior nasal swab specimens.

For in vitro diagnostic use only. For self-testing.

Carefully read the instructions before performing the test.

Materials Provided:

Kit Size	Contents
1T	1 Test Cassette, 1 Extraction Buffer Tube, 1 Disposable Swab, 1 Waste Bag, 1 Package Insert
5T	5 Test Cassettes, 5 Extraction Buffer Tubes, 5 Disposable Swabs, 5 Waste Bags, 1 Package Insert
20T	20 Test Cassettes, 20 Extraction Buffer Tubes, 20 Disposable Swabs, 20 Waste Bags, 1 Tube Holder, 4 Package Inserts


Materials Required But Not Provided: Timer

Scan the QR code in the guide or the packaging to access the guide in multiple languages and the test video on AusDiagnostics.care.




ausdiagnostics.care/resources


PREPARATION




1. Wash or sanitize your hands. Make sure they are dry before starting the test.

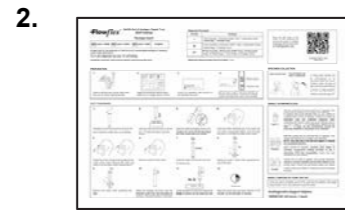

2. Read the instructions before using SARS-CoV-2 Antigen Rapid Test kit.

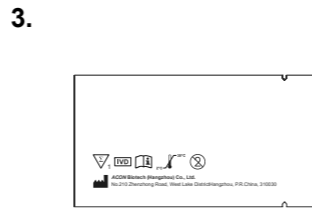

3. Check the expiration date printed on the cassette foil pouch.

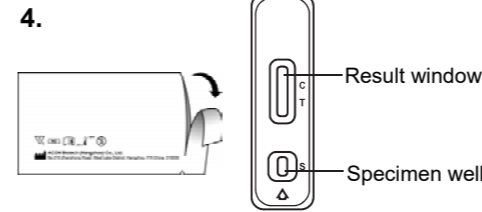

4. Open the pouch. Place the test cassette on a flat and clean surface. Check for the Result window and Specimen well on the cassette.

SPECIMEN COLLECTION

SELF COLLECTION




COLLECTION BY AN ADULT CAREGIVER




A nasal swab sample can be self-collected by an individual aged 18+ years. Children under 18 years of age should be performed by a parent or legal guardian. Do not use the test in children under the age of 2.


TEST PROCEDURE




1. Carefully remove the aluminum foil from the top of extraction buffer tube, avoid spilling.




2. Insert the tube into the hole on the kit box. (Or place the tube in the tube holder.)

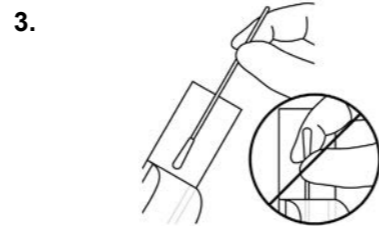


3. Open the swab packaging at stick end. **Caution: Do not touch the absorbent tip of the swab with your hands.**

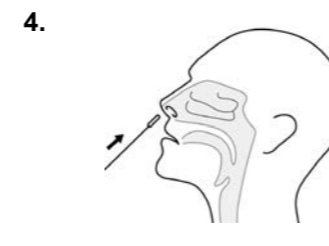


4. Insert the entire absorbent tip of the swab into one nostril. Using gentle rotation, push the swab less than 2.5 cm from the edge of the nostril.

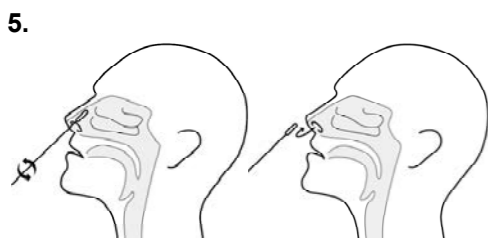


5. Rotate the swab 5 times brushing against the inside of the nostril. Remove the swab and insert it into the other nostril. Repeat step 4.

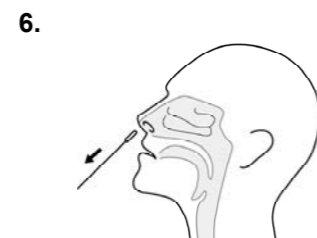


6. Remove swab from the nostril.

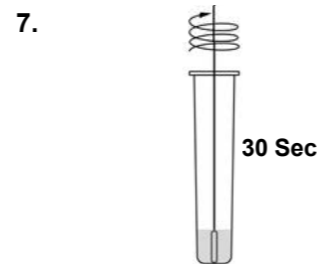


7. Insert the swab into the tube and swirl for 30 seconds.

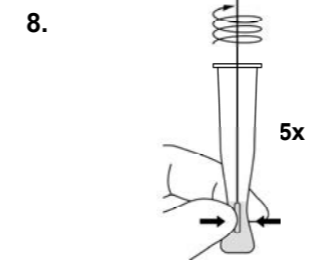


8. Rotate the swab 5 times while squeezing the side of the tube.



9. Remove the swab while squeezing the tube.



10. Attach the dropper tip firmly onto the extraction buffer tube. Mix thoroughly by swirling or flicking the bottom of the tube.

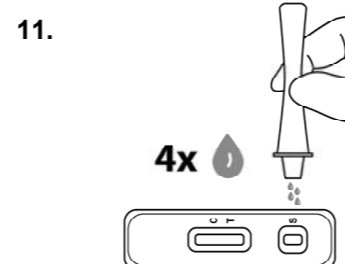


11. Gently squeeze the tube and dispense 4 drops of solution into the Specimen well.



15-30 min.


12. Read the result when the timer reaches 15-30 minutes. Do not read after 30 minutes.

RESULT INTERPRETATION




Negative

Only the control line (C) and no test line (T) appears. This means that no SARS-CoV-2 antigen was detected. A negative test result indicates that you are unlikely to currently have COVID-19 disease. Continue to follow all applicable rules and protective measures when contacting with others. There may be an infection even if the test is negative. **If it is suspected, repeat the test after 1 - 2 days, as the coronavirus cannot be precisely detected in all phases of an infection.**



Positive

Both the control line (C) and test line (T) appears. This means that SARS-CoV-2 antigen was detected. **NOTE: Any faint line in the test line region (T) should be considered positive.** A positive test result means it is very likely you currently have COVID-19 disease. Follow the relevant State or Territory health authority advice and regulation. Follow the local guidelines for self-isolation.



Invalid

Control line (C) fails to appear. Not enough specimen volume or incorrect operation are the likely reasons for an invalid result. Review the instructions again and repeat the test with a new cassette. If the test results remain invalid, contact your State or Territory Coronavirus testing services.

SAFELY DISPOSE OF YOUR TEST KIT

Once your test is complete, put all of the used test kit contents in the waste bag provided. Put in your general household waste.

AusDiagnostics Support Helpline:
1800951381 (24 hours, 7 days)

